



Medical Protective Clothing

As the professional manufacture, we would like to provide you Fealter® Medical Protective Clothing. Medical Protective Clothing Used for general isolation in outpatient department, ward and examination room, etc.

You can rest assured to buy Fealter® Medical Protective Clothing from our factory and we will offer you the best after-sale service and timely delivery.

Product name: Fealter® Medical Protective Clothing

Product number: 8010101

Intended use: Used for general isolation in outpatient department, ward and examination room, etc.


Product description: The material is made of 60% PP+40%PE non-woven fabric. The material has the characteristics of water resistance, blood permeation resistance, alcohol permeation resistance, high breaking strength, no peculiar smell, etc. It has the function of common isolation.

Product model: Siamese style

Product specification: 160 / S; 165/M 170 / L; 175/XL; 180 以 XL; 185/XXXL

According to your figure, choosing a suitable size of isolation gown to ensure there is enough space for convenient work

Speciflcations Company(cm)	Length	Bust	Sleeve length	Cuff
160/S	165	120	84	18
165/M	169	125	86	18
170/L	173	130	90	18
175/XL	178	135	93	18
180/XXL	181	140	96	18
185/XXXL	188	145	99	18

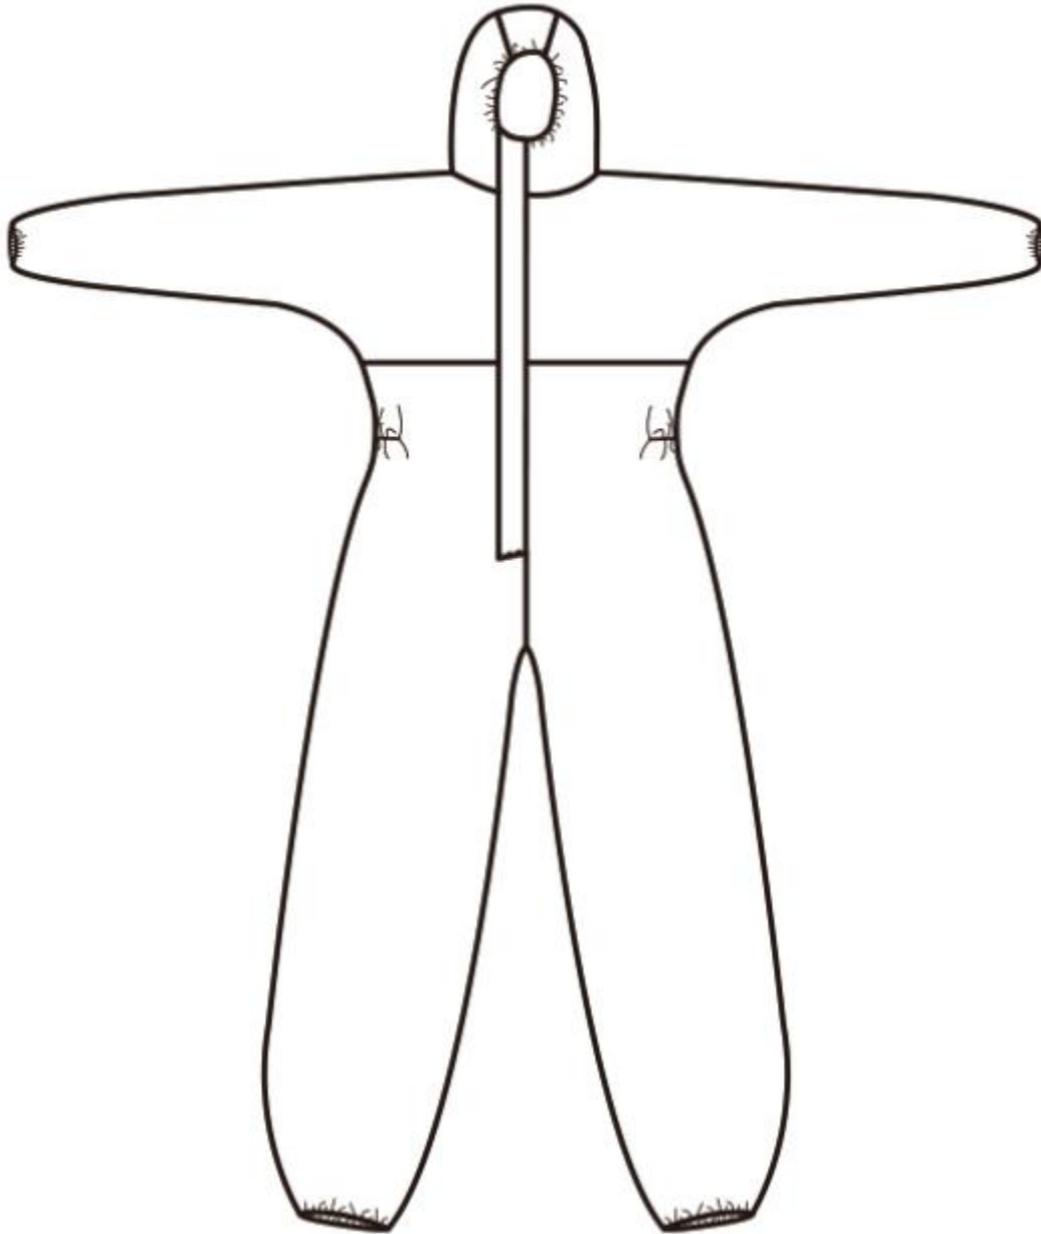

Implementation standard number EN14126: 2003+ ACI2004

Storage: It should be stored in a dry, ventilated and non-corrosive environment, away from fire and inflammables

Precautions:

1. Please strictly follow the usage and usage restrictions of this product when using it. Users should judge whether this product is suitable for specific occasions. If the usage exceeds the usage and usage restrictions of this product, we do not make any guarantee or assume any responsibility related to this.
 2. Please avoid direct sunlight.
 3. This product melts at 135 degrees Celsius. Please pay attention to keep away from open flames and heat sources when using it
 4. Not washing, washing will affect the protective effect.
 5. Do not iron, machine wash or dry clean.
 6. This product is for one-time use. Please dispose it properly according to relevant national regulations on pollutant disposal after use
- Manufacturer: Ningbo Snowwolf Outdoor Apparel Co., Ltd

Manufacturer : Ningbo Snowwolf Outdoor Apparel Co., Ltd .
Address : Gao Qiao Village , Gao Qiao Town , Haishu District , Ningbo City , Zhejiang Province . China
Tel:86-0574-87831668
 Date of production:See quality certificate for details.
 Product validity:Single use,non-sterile,storage pperiod is 3 years.
 The instruction was written on April 8th,2020.
 Please read the instructions before use.

- ANTI-PENETRATION OF ALCOHOL
- ANTI BLOOD SPLASH
- ANTI-BACTERIAL PARTICLES
- WATERPROOF



PROFESSIONAL TESTING



National Supervision and Inspection Center (Zhejiang) of Textile and Garments Quality
Ningbo Fibre Inspection Institute

TEST REPORT

Report No.: NFEW202004874 Issue Date:03/12/2020

Sample name: medical protective clothing
 Sample received date:03/12/2020
 Applicant: Ningbo Snowwolf Outdoor Apparel Co., Ltd
 Sample No.: White
 Sample Qty.: one piece
 Test items: listed as follows:

Test item	Test method	Standard Requirement	Result	Pass/Fail
Appearance quality		Protective clothing should be dry, clean, free of odour. Defects such as rashes, cracks and holes are not allowed on the surface of the fabric. Protective clothing connection parts can be stitched, glued and heat sealing methods. Folds of clothes should be sealed handle, which length should be 8-16 inches per line. Straps should be even, straight, and no jump of lines. Check or protruded parts such as heat sealing should be flat, sealed and no bubble. The zipper can't be exposed. The zipper puller should be self-locking	It is accord with standard requirement	Pass
	CB/T 3923.1-2013 GB/T 4746-2013 GB/T 4745-2012			
Breaking strength, N	GB/T 17323.3-2009	Warp : ≥45	85	Pass
Elongation at break, %	Standard specified by applicant	Warp : ≥25	32	Pass
		Warp : ≥15	79	Pass
Water resistance, kPa (before washing)	GB 19082-2009	Warp : ≥15	166	Pass
		Warp : ≥15	18.52	Pass
Spray rating, grade (before washing)		≥3	3	Pass
Water vapour transmission rate, g/m ² ·h (before washing)		≥2500	2408	Pass
Electrostatic properties (before washing)		Electric charge, μC/once/GB	8.1	Pass

Remark: The inspected items are determined according to the standard specified by applicant.
 Sample:



Approver: 

Add: Building F4, No.1588, Jiangnan Road, Hi-tech Zone, Ningbo, China Postcode:315045
 Tel:(+86)574-85331160 Email: nfe@nfi.com.cn
 Business Tel: 0574-90371020 <http://www.nfi.com.cn>

a