KINGSTAR

Anterior Nasal Covid-19 Self Test Rapid Antigen Test

As the professional manufacturers, KINGSTAR INC would like to provide you Anterior Nasal Covid-19 Self Test Rapid Antigen Test. Anterior nasal covid-19 self test rapid antigen test is used to detect the present of SARS-CoV-2 antigens in human anterior nasal swab specimens.

www.antigentestdevice.com

KINGSTAR INC is a professional leader China Anterior Nasal Covid-19 Self Test Rapid Antigen Test manufacturers with high quality and reasonable price. Welcome to contact us.

Product Introduction

Anterior nasal covid-19 self test rapid antigen test is intended for out-of-laboratory use, self-monitoring. The test results from the kits are for information purposes only and are not a substitutes for tests performed by healthcare professionals. An accurate diagnosis can only be made based on the patient's clinical symptoms and the results of other laboratory tests.

Product Parameter (Specification)

Test Cassette
Extraction buffer
Sterile swab
Instruction for Use
Biohazard Waste Bag

Anterior nasal covid-19 self test rapid antigen test

Product Feature and Application

Anterior nasal covid-19 self test rapid antigen test can be used by people themselves instead of medical staff. Its results come out quick which will save more time for us.

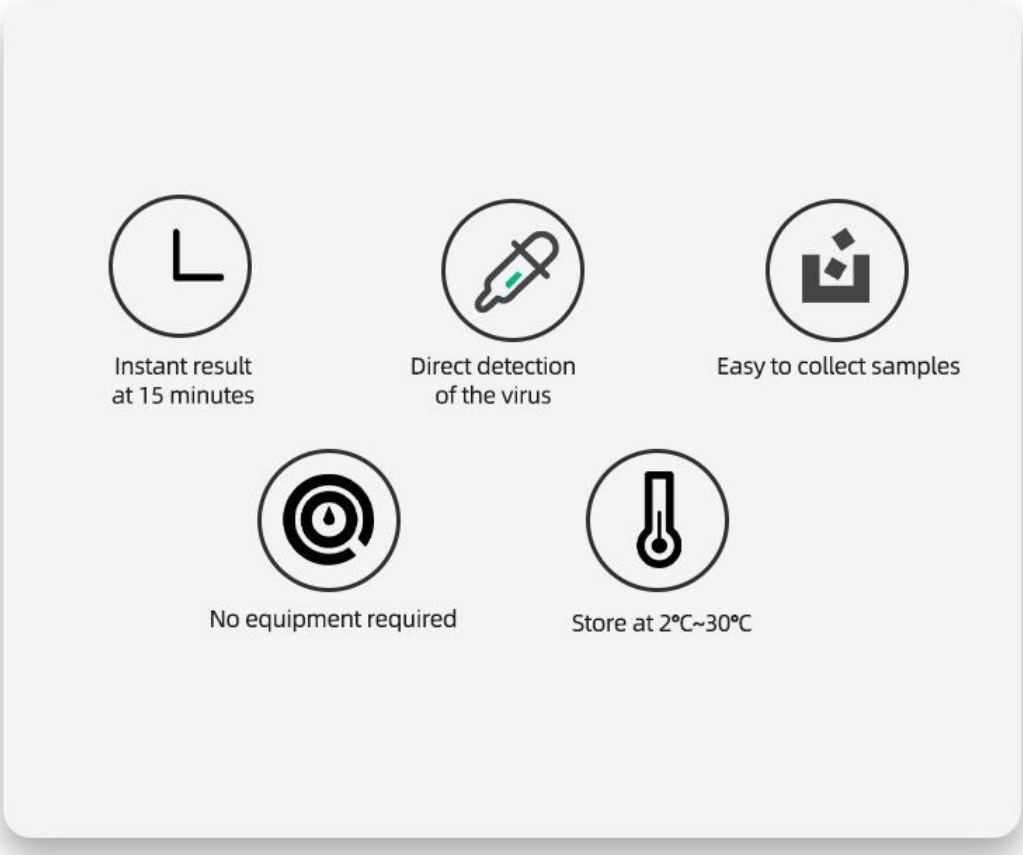

Test steps

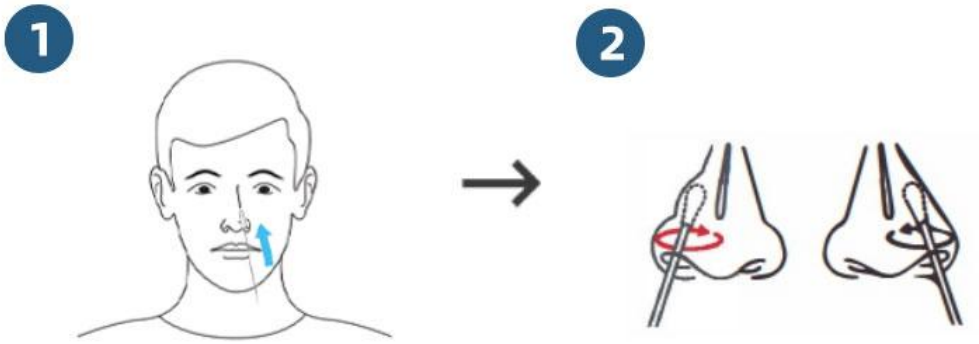

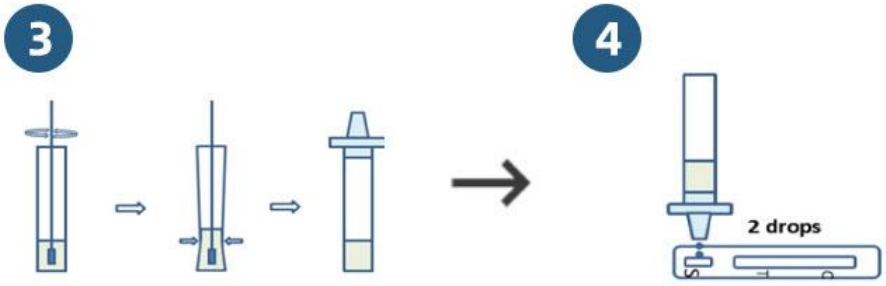

Product Details

Anterior nasal covid-19 self test rapid antigen test can get the result around 15 minutes. The result you read before 15 minutes are invalid. If no result is available after 20 minutes, it is recommended to repeat the test with a new test cassette.

5

Wait for 15 minutes and read the result.

Here are some examples of the colors of Tline.

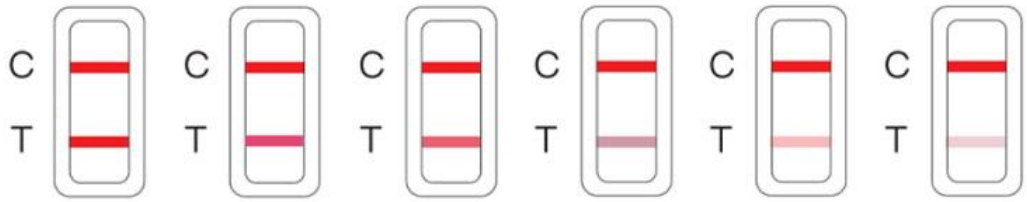

Positive

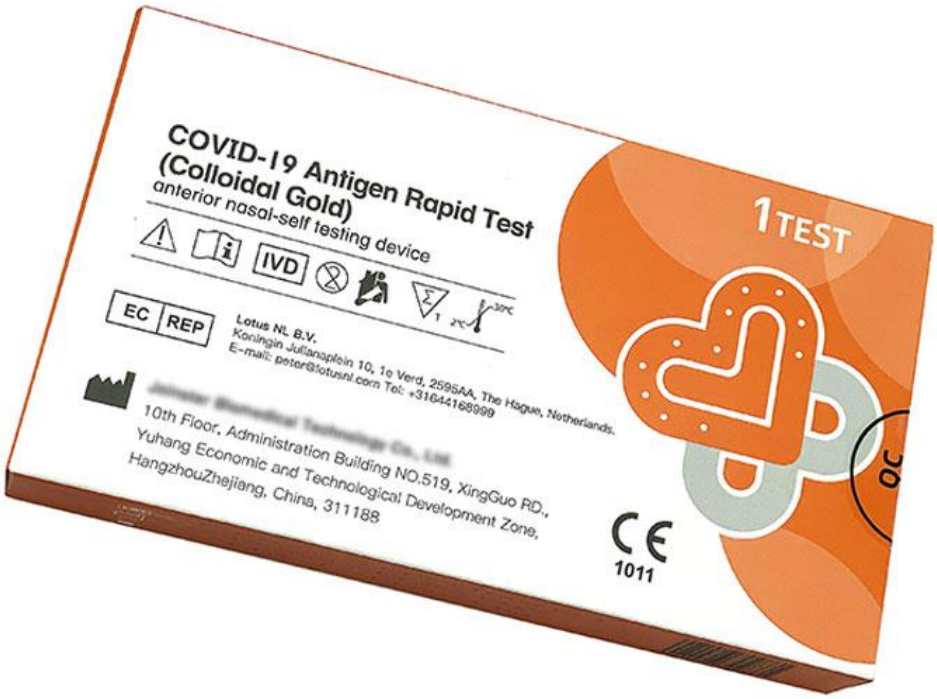
COVID-19 Antigen Rapid Test
(Colloidal Gold)
anterior nasal-self testing device
IVD
EC REP
Lotus NL B.V.
Koningin Julianaplein 10, 1e Verd, 2595AA, The Hague, Netherlands.
E-mail: peter@lotusnl.com Tel: +31644168999
10th Floor, Administration Building NO.519, XingGuo RD.,
Yuhang Economic and Technological Development Zone,
HangzhouZhejiang, China, 311188
CE
1011
1TEST
QC

1TEST
COVID-19 Antigen Rapid Test
(Colloidal Gold)
anterior nasal-self testing device
IVD
EC REP
Lotus NL B.V.
Koningin Julianaplein 10, 1e Verd, 2595AA, The Hague, Netherlands.
E-mail: peter@lotusnl.com Tel: +31644168999
10th Floor, Administration Building NO.519, XingGuo RD.,
Yuhang Economic and Technological Development Zone,
HangzhouZhejiang, China, 311188
CE
1011

COVID-19 Antigen Rapid Test
(Colloidal Gold)
anterior nasal-self testing device
DE: COVID-19 Antigen-Schnell-Selbsttest (kolloidales Gold)
FR: Autotest rapide de l'antigène COVID-19 (or colloïdal)
IT: Antigene COVID-19 Autotest rapido (oro colloidale)
ES: Autoprueba rápida del antígeno COVID-19 (oro coloidal)
PT: COVID-19 Autoteste rápido de antigeno (Ouro Coloidal)
NL: COVID-19 Antigeen Snelle Zelftest (Colloidaal Goud)
DK: COVID-19 Antigen Rapid Self Test (kolloidalt guld)
GR: COVID-19 γρήγορη αυτοδοκιμή αντιγόνου (κολλοειδής χρυσός)
HU: COVID-19 antigén gyors önellenőrzés (kolloid arany)
RO: Autotest rapid antigenul COVID-19 (aur coloidal)
PL: COVID-19 Antygen Szybki Test Samoistry (Złoto Koloidalne)
CZ: Rychlý autotest na antigen COVID-19 (koloidní zlato)
SI: COVID-19 Antigen Rapid Test (Koloidal Gold) nosni bris -
medicinski pripomoček za samotestiranje
LT: COVID-19 antigeno greitasis savarankiškas testas (koloidinis auksas)
BG: самостоятелен тест с антиген COVID-19 (колоидно злато)
HR: COVID-19 brzi antigenski test za samotestiranje (koloidno zlato)
SE: COVID-19 Antigen Snabbt självtest (kolloidalt guld)
FI: COVID-19 antigeenin nopea itsetesti (kolloidinen kulta)
1 тест | 1 testi | 1 δοκιμή | 1 testas | 1 Teste
1TEST

We have single serving, 5 servings 10 servings and 25 servings.

(If you have specific requirement, pls let us know.)

single serving

Warning and precaution

1. This kit is intended for in vitro diagnostic use only. Please read these instructions carefully before testing.
2. Use only the sample swab and extraction buffer provided in the package and do not substitute components from other kits for the specimen extract provided in this kit.
3. Strictly follow the instructions in this manual when performing the test.
4. Positive and negative predictive values are highly dependent on prevalence. When disease prevalence is low and SARS-CoV-2 is not or only minimally active, positive test

results are more likely to represent a false positive result. When disease prevalence is high, false negative results are more likely.
5. Compared to a SARS-CoV-2 RT-PCR test, this test is less sensitive when used to detect patient samples within the first five days of symptom onset.
6. Waste and excess samples generated during the test may be disposed of with household waste.
7. The contents of the desiccant pad included in the test cartridge package are toxic, do not consume.

Storage and stability

1. The test is stable for 2 years if all parts are stored in sealed pouches at +2°C to 30°C and the packaging of all devices is unopened and undamaged.
2. The test should be stored in the sealed pouch until use. Do not freeze the test and do not use it after the expiry date.
3. Please refer to the package for the date of manufacture and expiry date.

The following is the certificates of Anterior nasal covid-19 self test rapid antigen test.

EC DESIGN-EXAMINATION CERTIFICATE

Directive 98/79/EC on In Vitro Diagnostic Medical Devices, Annex III (6)

No. 7-038-306-2110

The **NEOEMKI National Medical Device Conformity Assessment and Certification LLC.** certifies that the following manufacturer's

[redacted]

with authorized representative in EU:

Lotus NL B.V.
Koningin Julianaplein 10, 1e Verd
2595AA The Hague, Netherlands

product's **COVID-19 Antigen Rapid Test (Colloidal Gold) anterior nasal - self testing device**

following model's

FGCOVG7100 1 test / kit
FGCOVG7200 5 tests / kit
FGCOVG7300 10 tests / kit
FGCOVG7400 25 tests / kit

design dossier conforms to the requirements of Directive 98/79/EC on in vitro diagnostic medical devices.

Registry number of the report on the examination of the design dossier: **NE/195/2021**

This certificate is valid until: **2024-05-26**

Issued by NEOEMKI LLC. as a Notified Body with identification number 1011.

Budapest, 2021-10-19

László Imre
Managing Director

EMKI 2785

The authenticity and validity of the certificate are verifiable at NEOEMKI LLC.

neoEMKI Nemzeti Orvostechnikai Eszköz Megfelelőségértékelő és Tanúsító Kft.
neoEMKI National Medical Device Conformity Assessment and Certification LLC.

H-1097 Budapest, Albert Flórián út 3/A, tel: +36 20 268 75 95, e-mail: cert@emki.hu
www.emki.hu